

# Boston Brace Night Shift Order Form Instructions

Reminder – this form is for the technicians and goes with the flow of fabrication. All items on this form need to be completed to ensure customer service and manufacturing are able to fabricate the desired orthosis.

PLEASE DO NOT use this as your clinical note.

This form is for the fabrication of the Boston Brace Night Shift orthosis.

All items in bold are required and represent the recommended standard.

The Boston Sensor is standard of care for our scoliosis patients. Discuss this with the parents/caregiver.

## Demographics:

### Boston Brace Nightshift Order Form

Date: _____	Due Date: _____	PO #: _____	Contact: _____
Ship To: _____	Ship Via: _____	Email: _____	
Address: _____	Account #: _____	Phone: _____	
City: _____ State: _____ Zip: _____	<input type="checkbox"/> Previous Nightshift Wearer	Scan Label: _____	

Customer service uses this section to initiate the fabrication process. All of the above is entered into our system. In the event we need to contact you, the treating orthotist, or if you have a question on the fabrication, having this information entered allows for easy retrieval.

## Previous Wearer:

Previous Nightshift Wearer

Let us know if the patient has worn a nighttime brace before. If so, our technicians will notify you if there is a design change.

## Scan label:

Scan Label: \_\_\_\_\_

Scan label is required to make sure the correct scan is modified.

Captevia: File name is auto-populated. The file will include both scans if taking a bivalve scan.

Techmed: File name is auto-populated within Boston O&P App. The file will include both scans if taking a bivalve scan.

Laser scanner: Patient's first initial, last name; scan number; clinicians' initials;  
the word scoli; date of scan

i.e. patient John Smith is seeing clinician Jane Doe on April 1, 2020 for his first brace.

Scan Label: jsmith#1jdscoli04012020

Bivalve scan: Follow the sequence above and add \_ant and \_post after the date

Anterior section: jsmith#1jdscoli04012020\_ant  
Posterior section: jsmith#1jdscoli04012020\_post

**Patient Name, Age, Sex, Height, Weight, Diagnosis:**

Patient Name: _____	Ht: _____	ft	in	Wt: _____	lbs
Age: _____	Sex: _____	Diagnosis: Idiopathic Scoliosis			

We will keep a secondary record for you showing the patient’s age, sex, height and weight as well as the diagnosis. This information may assist in justifying a new orthosis.

Make sure all information is legible.

Age and Sex are needed to complete our records in the event you need the manufacturing record. Height is broken down into feet and inches to ensure proper record keeping. Weight is requested to be in pounds. Diagnosis is needed to complete records.

**Required	Lumbar/TL	Thoracic
Convexity	<input type="checkbox"/> Left <input type="checkbox"/> Right	<input type="checkbox"/> Left <input type="checkbox"/> Right
Apical Vertebra		
Cobb Angle		
Scoliometer Reading		


The above chart must be fully completed to monitor outcomes and provide guidance for shift/push magnitudes. Indicate the side of the curve convexity (left or right). Please indicate the numerical values for Apical vertebra, Cobb angle, and scoliometer reading in the designated box. Apical vertebra: denote the apical vertebra for the curve(s) (Example- T9 or L3). Cobb angle: indicate the angle of the selected curve(s) in degrees (Example: 35deg). Scoliometer reading: document your findings from the scoliometer reading to determine the degree of rotation of the curve(s) (Example: 9 deg). Both the Cobb angle measurement and the scoliometer reading will help to determine the push magnitude built into the brace

## Anatomical Measurements:

All Circumferential, ML, AP and linear anatomical measurements are required. We recommend taking these measurements in standing.


### Anatomical Measurements

All measurements required in standing

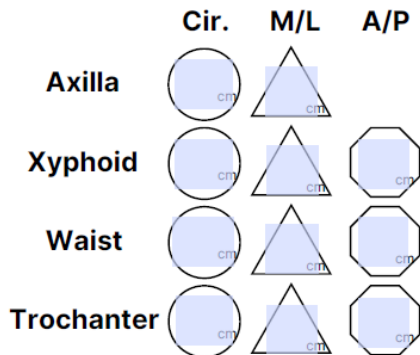

### Shape Capture

Scan  Measure Only  Cast

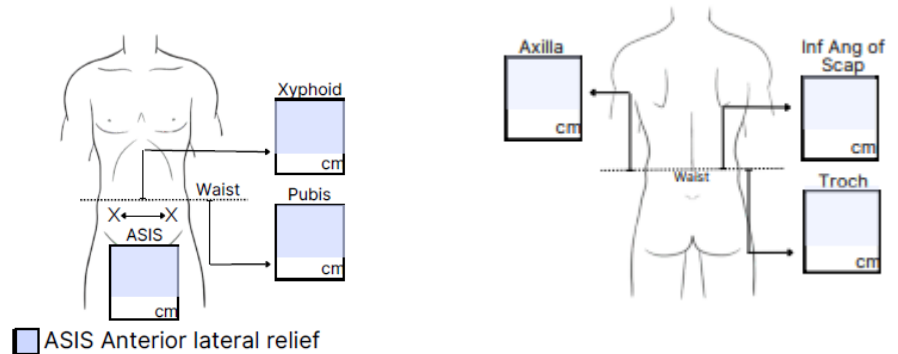

## Shape Capture

Indicate the method used to capture the patient's shape. This lets customer service know if they need to contact you or not if a scan is not attached to the order.

### Shape Capture

Scan  Measure Only  Cast

## Brace Design

### Brace Design

#### Abdominal Shape

Neutral  
 Other: \_\_\_\_\_

#### Plastic

1/8" Copoly  
 Other: \_\_\_\_\_

#### Straps

White  
 Black

#### Liner

1/4" Aliplast  
 Other: \_\_\_\_\_

#### Lordosis

15 degrees  
 Other: \_\_\_\_\_

#### Transfer

1st \_\_\_\_\_  
 2nd \_\_\_\_\_

#### Tongue 1/16" PE

Attached  
 Send

Standard options are prefilled, if you wish something outside of the standard, please uncheck the standard box and check the other and fill in the text box.

## Abdominal Shape:

We do not provide any abdominal compression. Neutral would be a flat/convex abdomen dictated by the patient's measurements/shape.

Abdominal relief is relative to the patient's size. If you would like a relief, use the terms small/medium/large to provide guidance to our CAD technicians. Provide AP measurements at the xyphoid, waist and pubis if a relief is requested.

#### **Lordosis:**

The standard is 15° lordosis. The goal is sagittal balance, so minor adjustments may be made in CAD. Let us know the desired lordosis for your patient if other than 15°.

#### **Plastic:**

1/8-inch co-poly and ¼ inch aliplast are the standard plastic/liner for the Night Shift. If your patient requires something different, indicate the thickness and plastic/foam type required.

It is standard for the tongue to be attached, please indicate if you prefer it to be sent separate.

#### **Transfer:**

Patients may choose their transfer using the Boston O&P transfer tool.

(<https://www.bostonoandp.com/transfers/brace/>). Write the brace *transfer name* in this section as well as a backup choice. Two transfers cannot be combined.

#### **Straps:**

Standard straps are white. Indicate the color of the straps requested by the patient. Strap transfers are no longer an option here as they decrease the life and integrity of the straps.

#### **Liner:**

¼ inch Aliplast lining is the standard. Indicate both the foam type and thickness if ordering outside of the standard.

#### **Tongue:**

A 1/16 inch attached polyethylene tongue is standard. If you wish to have the tongue unattached, click the send box.

#### **Boston Sensor:**

### **Boston Sensor**

---

Send Sensor

Sensor Hole

The Boston Sensor adherence monitor is standard of care for the Boston Brace 3D. Boston Sensors may be transferred to a patient's subsequent brace.


Indicate if a Sensor is to be sent with the brace.

If the patient has a Sensor, and just needs to have the hole drilled into the brace, check Sensor Hole

## CAD Design Section: Optional

**CAD Design Section** (Optional)

<u>Lumbar</u> <input type="checkbox"/> Left <input type="checkbox"/> Right Push: <input type="text"/> Shift: <input type="text"/> Pad: <input type="checkbox"/> 1/2" <input type="checkbox"/> 1/4" <input type="checkbox"/> Sym	Apex T12- L1 <u>Thoracolumbar</u> <input type="checkbox"/> Left <input type="checkbox"/> Right Push: <input type="text"/> Shift: <input type="text"/> Pad: <input type="checkbox"/> 1/2" <input type="checkbox"/> 1/4"	<u>Thoracic Extension</u> <input type="checkbox"/> Left <input type="checkbox"/> Right Push: <input type="text"/> Shift: <input type="text"/> Pad: <input type="checkbox"/> 1/2" <input type="checkbox"/> 1/4" <input type="checkbox"/> Sym	<u>Axilla</u> <input type="checkbox"/> Left <input type="checkbox"/> Right  <u>Trochanter</u> <input type="checkbox"/> Left <input type="checkbox"/> Right Pad: <input type="checkbox"/> 1/4"
--	---	--	--



The brace design is determined by the x-ray blueprint and the patient presentation. This section is optional. Our CAD technicians will complete.

## Finish Heights

**Finished Heights** \*from waist

Xyphoid: <input type="text"/> cm	Axilla: <input type="text"/> cm
Thoracic Ext: <input type="text"/> cm	Trochanter: <input type="text"/> cm

All finished heights are to be in CM and are taken from the waist.

## Scoli T's:

**Scoli Tees**  
 Single  Double Qty:

Indicate how many Scoli Tees you would like sent with your orthosis and if you prefer single or double underarm flaps. T-shirts do not have a front or back, so a single axilla can be left or right. The size is determined from the submitted measurements.

## Notes

**Notes:**

In the event a special request is made by the patient, or there is some unique anatomy or brace design needed that is not captured in the above sections, the notes section is where you may document this information.